# Installation Instructions

## 9A31600* Oral Surgery Armboard w/Mtg. Rails
## 9A31700* Armboard Mounting Rails only

### Intended Use
To secure patient's arm during medical procedures.

### Kit Components *(9A31600*)*

| *Description* | *Part Number* | *Qty* |
|---|---|---|
| Armboard | 029-3025-00 | 1 |
| LH Mounting Rail | 030-1368-00 | 1 |
| RH Mounting Rail | 030-1367-00 | 1 |
| Knob | 016-0304-00 | 2 |

### Kit Components *(9A31700*)*

| *Description* | *Part Number* | *Qty* |
|---|---|---|
| LH Mounting Rail | 030-1368-00 | 1 |
| RH Mounting Rail | 030-1367-00 | 1 |
| Knob | 016-0304-00 | 2 |

### Mounting Rail Installation

**NOTE**
Retain screws (1) and spacers (3) to install armboard mounting rails.

(1) Remove two screws (1, Figure 1), two accessory rails (2) and two spacers (3). Repeat to remove other rail.

**NOTE**
Armboard mounting rails should angle inward, toward table top as shown in Figure 1.

(2) Position armboard mounting rail (4) and two spacers (3); then secure with two screws (1). Repeat to install other rail.




MA619300i

**Figure 1. Mounting Rail Installation**

© Midmark Corporation - 2003

## Armboard Installation

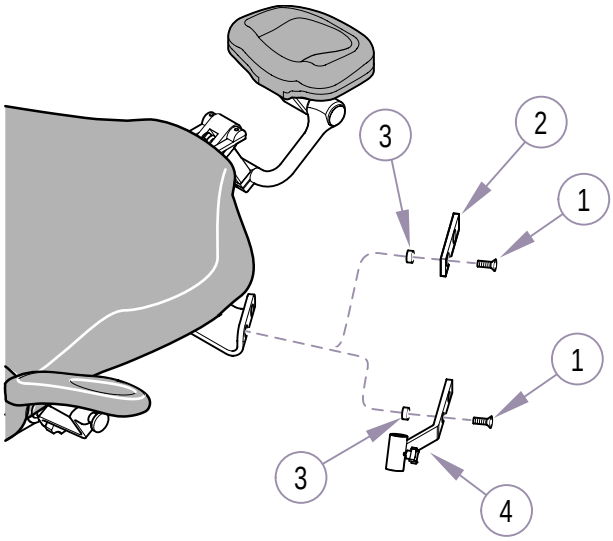**NOTE**
If installing an armboard other than the 9A31600*, remove the rail clamp, then follow this procedure.

(1) Remove screw (1, Figure 2) and washer (2) from shaft of armboard (3).

(2) Slide shaft of armboard (3) into mounting rail socket (4).

(3) Install washer (2) and screw (1) into shaft of armboard (3).

**NOTE**
Position armboard so that knob tightens against flat side of shaft.

(4) Move armboard (3) to desired height, then tighten knob (5).

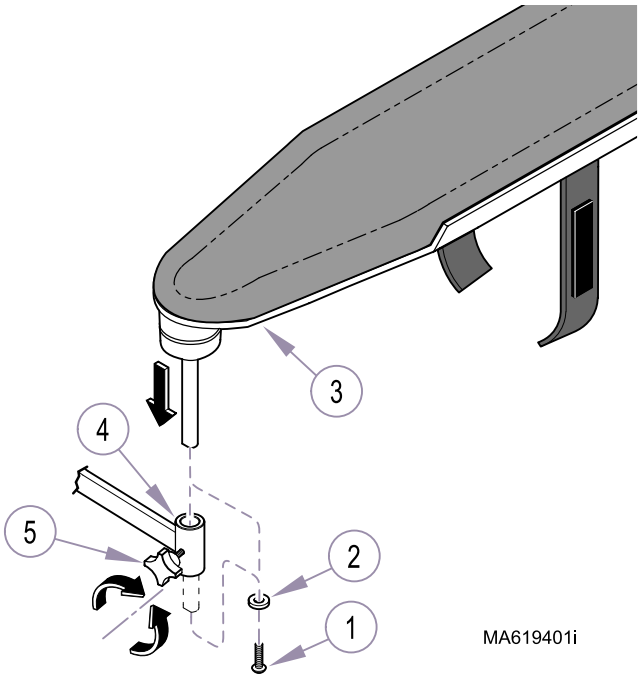


**Figure 2. Armboard Installation**

## Handle / Locking System Adjustments

**CAUTION**
If armboard does not lock securely in place, perform the following adjustment. Failure to do so may result in armboard movement during procedures.

***A. To adjust handle tension...***

(1) Using a 2.5mm allen wrench, loosen / tighten two screws (1, Figure 3) as necessary.

***B. To adjust locking system...***

(1) Using a 3mm allen wrench, loosen locking screw (2, Figure 3).

(2) Using a 3mm allen wrench, loosen / tighten screw (3) as necessary.

(3) Check for proper operation. Repeat as necessary

(4) Tighten locking screw (2).

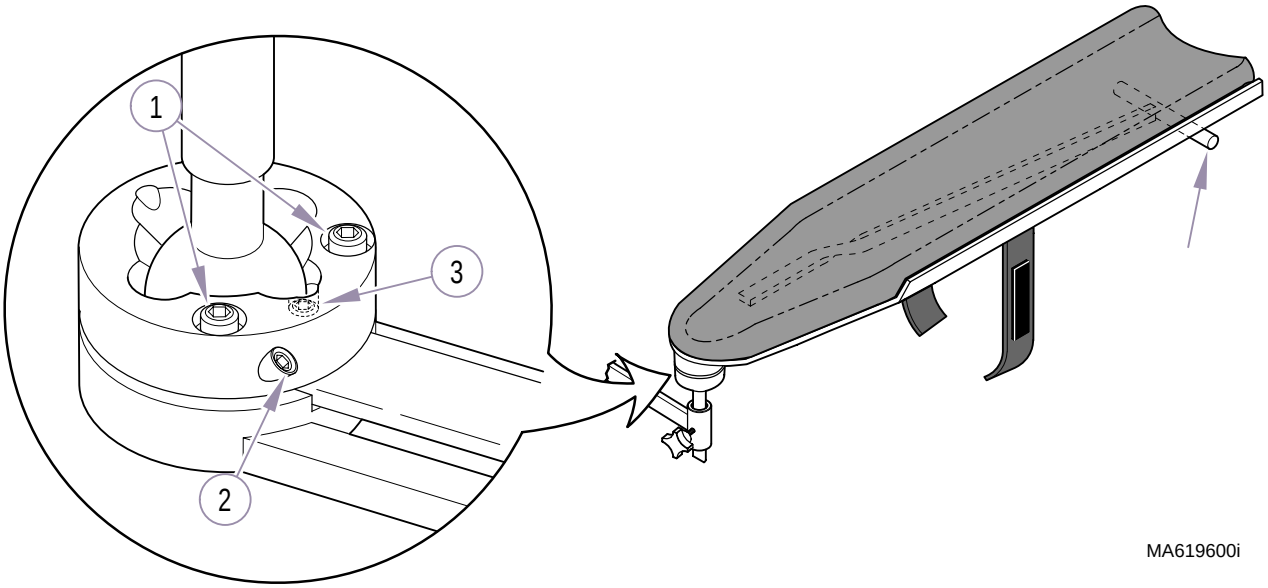


**Figure 3. Handle / Locking System Adjustment**

© Midmark Corporation - 2003